

D-SPECT-L™ Cardiac Imaging System

TECHNICAL SPECIFICATIONS

Detector Specifications

Intrinsic Spatial Resolution	
FWHM in UFOV	NA
FWTM in UFOV	NA
<i>*D-SPECT uses Integrated Collimators*</i>	

Intrinsic Spatial Linearity

Differential in UFOV	NA
Integral in UFOV	NA
<i>*Linearity defined by pixelated structure with NO drifts</i>	

Extrinsic Energy Resolution

FWHM at 140keV	≤6.2%
----------------	-------

Intrinsic Energy Resolution

FWHM at 140keV	NA
----------------	----

Extrinsic Uniformity

Differential in UFOV	<3%
Integral in UFOV	<4%

Intrinsic Uniformity

Differential in UFOV	NA
Integral in UFOV	NA
<i>*D-SPECT uses Integrated Collimators*</i>	

Max Count Rate with Scatter

(Per camera with <5% count Loss)	>900,000 cps
----------------------------------	--------------

Reconstructed Spatial Resolution

FWHM with Scatter at 15cm	5.0 mm
---------------------------	--------

ECG Gating

Number of Frames per R-R	8 or 16
Automatic Beat Centering	Yes
Integrated ECG	Yes



Detector Properties

Detector Technology	Solid State
Detector Type	Pixelated Crystals
Collimator Type	Tungsten
Number of Detectors	6
Camera Field-of-View(FOV)	15.74 cm x patient adjustable
Detector Field-of-View(UFOV)	15.74 x 3.94 cm (6.2 x 1.6 in)
Number of Pixels per Detector	1024
Total Number of Pixels	6144
Detector Range of Motion	>110°
Pixel Size	2.26mm x 2.26 mm
Energy Range	40 - 170 keV
Lead Shielding	175 keV

Crystal Properties

Crystal Material	CZT (Cadmium Zinc Telluride)
Crystal Type	Semi-Conductor
Decay Time	300ns
Detection Efficiency	80% @140keV
Crystal Thickness	5.0 mm (0.2 in)

Patient Chair

Max Patient Weight (Static)	454kg (1000 lb)
Max Patient Weight (Dynamic)	240g (529 lb)
Lowest chair position from floor	60cm (23.62 in)
Highest chair position from floor	90cm (35.43 in)

Footprint and Weight


Height	190 cm (74.8 in)
Depth	216 cm (85.04 in)
Width	173 cm (68.11 in)
Weight	620 kg (1367 lb)
Floor Loading (No Patient)	564 kg/m ² (115 lb/ft ²)



PHYSICAL, ENVIRONMENTAL, AND POWER SPECIFICATIONS

System Component	Condition	Ambient Temperature	Relative Humidity (Non-Condensing)
D-SPECT-L Cardiac Scanner	Operation	15 -24° C	30 -65 %
		59 -75° F	
	Max Temp Change Rate	3° C per hour	
		5.4° F per hour	
	Storage and Transportation	0 - 30° C	30 -65 %
	32 -86° F		
	Heat Dissipation Handling	6800 BTU/Hr	

D-SPECT-L System Configuration	Power (VA)	Nominal Input Voltage (VAC)	Allowed Input Voltage (VAC)	Frequency
With 120V UPS	1440 VA	120VAC	95-151 VAC	60Hz
With 230V UPS	1440 VA	230 VAC	181-290 VAC	50-60 Hz

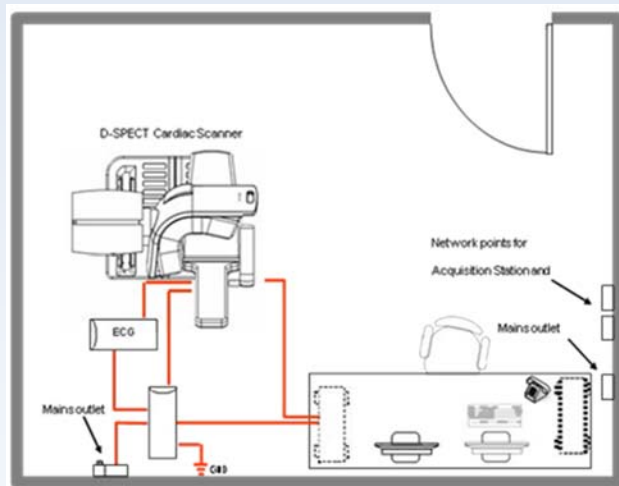

The D-SPECT-L has a small footprint that easily fits into compact spaces
 Minimum room requirements for upright imaging – 9'5" x 8'8"
 Minimum room requirements for supine imaging – 9'5" x 11'

Spectrum Dynamics Medical, Inc.
 301 N. Cattlemen Rd. Suite 109
 Sarasota, FL 34232 USA
 Tel 941 256 3660
 Fax 941 256 3662
 info@spectrum-dynamics.com
www.spectrum-dynamics.com

Spectrum Dynamics Medical HK LTD
 5 Canton Road Suite 1729A
 Ocean Center
 Tsim Sha Tsui, Kowloon, Hong Kong
 Tel +852 580 14151
 Fax +852 580 14146

Spectrum Dynamics Medical SA
 Rue de Lausanne, 31
 1110 Morges, Switzerland
 Tel +41 21 544 4710
 Fax +41 21 544 4711

Spectrum Dynamics Medical reserves the right to make changes in specifications without notice or warning
 D-SPECT® is a registered trademark of Spectrum Dynamics Medical.
 ©2017 All rights reserved.